



Test Report/ Certificate of Analysis

Date of Report June 17, 2026
To: MHS Longevity
From: AxisPharm, LLC
Certificate ID Number: 17Jun2026-01

Results reported by: Lab Technician
Ning Yang

Review/Approved by:

QA Director
Dawei Yue


Sample Received: Date: 06/04/2026
Receiving Condition: ☒ Acceptable ☐ Other: _____
Storage Condition: ☐ Room temperature ☐ -20°C ☐ -80°C
☒ Other: __ 0 °C ____

Sample Name: Retatrutide Black 20mg; Brand Name: MHS
Longevity; Lot#: NA ; MFD: NA; BBD: NA
Method(s): LCMS and LAL Endotoxin Assay

Procedure(s): Laboratory Activity Date: 06/11/2026

Results:

Sample

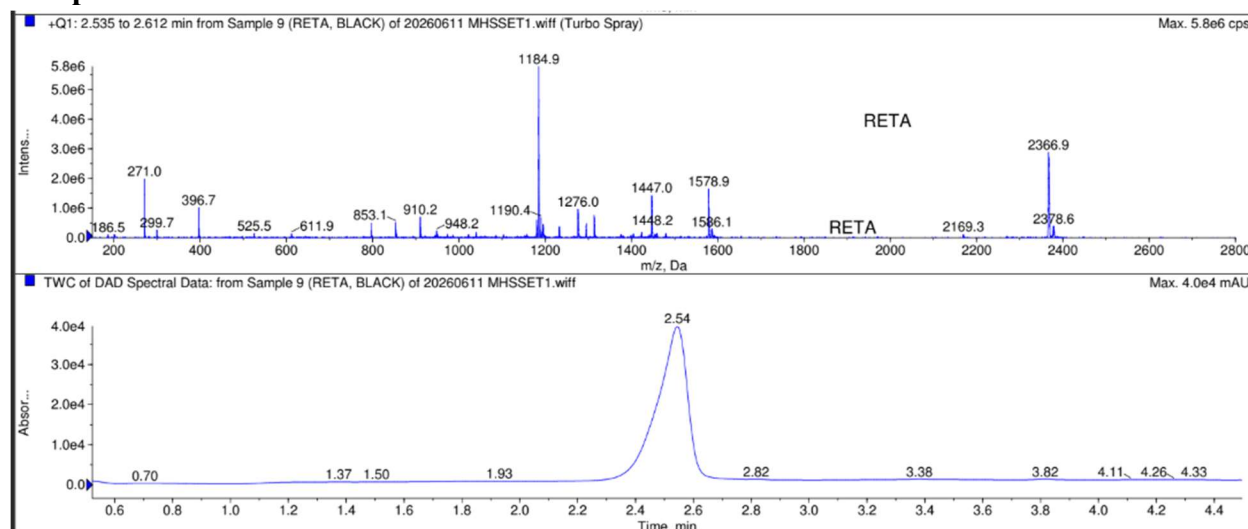

AxisPharm, LLC

Results only apply to tested Research Use Only samples within Test Report as received. Not for use in humans or animals. Analytical data apply only to the batch tested and do not indicate suitability for diagnostic or therapeutic use. Any unauthorized alteration, reproduction, or relabeling of this COA renders it invalid.



Test Report/ Certificate of Analysis

Sample Name	Net Weight Measured	MW (g/mol)	Detected	UV Purity (220nm) (%)
Reta BLK 20mg	19.5mg	4731.33	2366.9[M+2H], 1578.9[M+3H]	99.5

Endotoxin Results:

Sample Name	Endotoxin Testing Value (EU/mg)
Reta BLK 20mg	0.051

Preservatives, salts and sugars that serves as fillers in injectables are not considered as impurities. 19.5mg retartrutide is detected by UV and mass spec with purity of 99.5%.